

2018

# Clinical evaluation of the Cepheid Xpert TV assay for detection of *Trichomonas vaginalis* with prospectively collected specimens from men and women

C-A. D. Burnham

*Washington University School of Medicine in St. Louis*

H. Reno

*Washington University School of Medicine in St. Louis*

et al

Follow this and additional works at: [https://digitalcommons.wustl.edu/open\\_access\\_pubs](https://digitalcommons.wustl.edu/open_access_pubs)

---

## Recommended Citation

Burnham, C-A. D.; Reno, H.; and et al, "Clinical evaluation of the Cepheid Xpert TV assay for detection of *Trichomonas vaginalis* with prospectively collected specimens from men and women." *Journal of Clinical Microbiology*.56,2. e01091-17. (2018).  
[https://digitalcommons.wustl.edu/open\\_access\\_pubs/6756](https://digitalcommons.wustl.edu/open_access_pubs/6756)

This Open Access Publication is brought to you for free and open access by Digital Commons@Becker. It has been accepted for inclusion in Open Access Publications by an authorized administrator of Digital Commons@Becker. For more information, please contact [engeszer@wustl.edu](mailto:engeszer@wustl.edu).



# Clinical Evaluation of the Cepheid Xpert TV Assay for Detection of *Trichomonas vaginalis* with Prospectively Collected Specimens from Men and Women

Jane R. Schwebke,<sup>a</sup> C. A. Gaydos,<sup>b</sup> T. Davis,<sup>c</sup> J. Marrazzo,<sup>a</sup> D. Furgerson,<sup>d</sup> S. N. Taylor,<sup>e</sup> B. Smith,<sup>f</sup> L. H. Bachmann,<sup>g</sup> R. Ackerman,<sup>h</sup> T. Spurrell,<sup>i</sup> D. Ferris,<sup>j</sup> C.-A. D. Burnham,<sup>k</sup> H. Reno,<sup>k</sup> J. Lebed,<sup>l</sup> D. Eisenberg,<sup>m</sup> P. Kerndt,<sup>n</sup> S. Philip,<sup>o</sup> J. Jordan,<sup>p</sup> N. Quigley<sup>q</sup>

<sup>a</sup>Department of Medicine, University of Alabama at Birmingham, Birmingham, Alabama, USA

<sup>b</sup>Johns Hopkins University, Baltimore, Maryland, USA

<sup>c</sup>Indiana University School of Medicine, Indianapolis, Indiana, USA

<sup>d</sup>Planned Parenthood Mar Monte, San Jose, California, USA

<sup>e</sup>Louisiana State University Health Sciences Center, New Orleans, Louisiana, USA

<sup>f</sup>Planned Parenthood Gulf Coast, Houston, Texas, USA

<sup>g</sup>Wake Forest University Health Sciences, Winston-Salem, North Carolina, USA

<sup>h</sup>Comprehensive Clinical Trials, W. Palm Beach, Florida, USA

<sup>i</sup>Planned Parenthood of Southern New England, New Haven, Connecticut, USA

<sup>j</sup>Augusta University, Augusta, Georgia, USA

<sup>k</sup>Washington University in St. Louis, St. Louis, Missouri, USA

<sup>l</sup>Planned Parenthood Southeastern PA, Philadelphia, Pennsylvania, USA

<sup>m</sup>Planned Parenthood St. Louis Region, St. Louis, Missouri, USA

<sup>n</sup>University of Southern California, Los Angeles, California, USA

<sup>o</sup>San Francisco Public Health, San Francisco, California, USA

<sup>p</sup>George Washington University School of Public Health, Washington, DC, USA

<sup>q</sup>Geneuity, Maryville, Tennessee, USA

**ABSTRACT** Trichomoniasis is the most prevalent curable sexually transmitted disease (STD). It has been associated with preterm birth and the acquisition and transmission of HIV. Recently, nucleic acid amplification tests (NAAT) have been FDA cleared in the United States for detection of *Trichomonas vaginalis* in specimens from both women and men. This study reports the results of a multicenter study recently conducted using the Xpert TV (*T. vaginalis*) assay to test specimens from both men and women. On-demand results were available in as little as 40 min for positive specimens. A total of 1,867 women and 4,791 men were eligible for inclusion in the analysis. In women, the performance of the Xpert TV assay was compared to the patient infected status (PIS) derived from the results of InPouch TV broth culture and Aptima NAAT for *T. vaginalis*. The diagnostic sensitivities and specificities of the Xpert TV assay for the combined female specimens (urine samples, self-collected vaginal swabs, and endocervical swabs) ranged from 99.5 to 100% and 99.4 to 99.9%, respectively. For male urine samples, the diagnostic sensitivity and specificity were 97.2% and 99.9%, respectively, compared to PIS results derived from the results of broth culture for *T. vaginalis* and bidirectional gene sequencing of amplicons. Excellent performance characteristics were seen using both female and male specimens. The ease of using the Xpert TV assay should result in opportunities for enhanced screening for *T. vaginalis* in both men and women and, hopefully, improved control of this infection.

**KEYWORDS** NAAT, diagnosis, female, male, trichomonas

Received 20 July 2017 Returned for modification 17 August 2017 Accepted 11 October 2017

Accepted manuscript posted online 22 November 2017

**Citation** Schwebke JR, Gaydos C, Davis T, Marrazzo J, Furgerson D, Taylor SN, Smith B, Bachmann LH, Ackerman R, Spurrell T, Ferris D, Burnham C-AD, Reno H, Lebed J, Eisenberg D, Kerndt P, Philip S, Jordan J, Quigley N. 2018. Clinical evaluation of the Cepheid Xpert TV assay for detection of *Trichomonas vaginalis* with prospectively collected specimens from men and women. J Clin Microbiol 56:e01091-17. <https://doi.org/10.1128/JCM.01091-17>.

**Editor** Michael J. Loeffelholz, University of Texas Medical Branch

**Copyright** © 2018 Schwebke et al. This is an open-access article distributed under the terms of the [Creative Commons Attribution 4.0 International license](https://creativecommons.org/licenses/by/4.0/).

Address correspondence to Jane R. Schwebke, jschwebk@uabmc.edu.

D. Furgerson met authorship criteria but was unreachable for final approval of the byline and article.

*Trichomonas vaginalis* is a flagellated protozoan parasite that causes genitourinary infections in women and men. It is the most prevalent curable sexually transmitted disease (STD) and is easily treated with inexpensive antibiotics (1, 2). Trichomoniasis causes distressing symptoms like vaginal discharge and irritation in women and urethritis in men (3, 4). It is also significantly associated with an increased risk of preterm birth and the acquisition and transmission of STDs, including HIV, as well as being associated with infertility (5–8). Currently, however, there is no national control program for this infection. Until recently, the tests available for detection of the parasite were relatively insensitive (direct microscopy and antigen detection) or not widely available (culture) (9, 10). The advent and FDA clearance of nucleic acid amplification tests (NAAT) for diagnosis of *T. vaginalis* in women (urine [UR] samples, endocervical swab [ES] specimens, vaginal swab [VS] specimens, and patient-collected vaginal swab [PC-VS] specimens) has greatly improved our diagnostic capability, but until now there was no FDA-cleared test for detection of *T. vaginalis* in male urine samples (11). The GeneXpert system (Cepheid, Sunnyvale, CA) is already used to diagnose other STDs, such as *Neisseria gonorrhoeae* and *Chlamydia trachomatis* (12). We now report on the performance of this assay for the detection of *T. vaginalis* in specimens from women and men.

## MATERIALS AND METHODS

This multicenter study evaluated test performance in prospectively collected first-catch urine (UR) samples from both women and men, endocervical swab (ES) specimens, clinician-collected vaginal swab (CC-VS) specimens, and patient-collected vaginal swab (PC-VS) specimens in a clinical setting. The sites participating in this study were academic medical centers, STD clinics, family planning clinics, public health departments, and clinical trial offices. The sites were located across the United States, including the West Coast, the Midwest, Southern states, and the East Coast. Subjects were eligible for enrollment regardless of the presence or absence of genital symptoms. Seventeen diverse geographic sites participated in collection of the specimens. Institutional Review Board approval was obtained for each of the collection sites.

To be eligible for study enrollment, participants needed to be sexually active,  $\geq 14$  years of age, and provide informed consent and minor assent if needed. Subjects were excluded if they had been previously enrolled in the study, had received antimicrobial therapy within 21 days prior to enrollment, had undergone a hysterectomy, or had urinated less than 1 h prior to specimen collection. Female study participants were classified as symptomatic if they reported any of the following symptoms: itching, burning, redness, soreness, or irritation of the genitals, unusual odor, abnormal vaginal discharge, coital pain, and/or dysuria. Males were classified as symptomatic if they reported any of the following signs and/or symptoms: urethral discharge, dysuria, or urethral itching or burning, burning after ejaculation, and/or dysuria. Study participants not reporting any of the above symptoms were classified as asymptomatic.

The following samples were collected from females: one PC-VS specimen (collected in a clinical setting) for testing by the Xpert TV assay, followed by two CC-VS specimens for testing by the InPouch TV culture-based method (BioMed Diagnostics, White City, OR) and the Aptima TV NAAT (Hologic, Bedford, MA) (specimens alternated), three ES specimens (the first swab for InPouch, while the second and third swabs were alternated for Aptima and Xpert assays), and 35 to 50 ml of first-catch UR for InPouch, Xpert, and Aptima assays. For males, 35 to 50 ml of first-catch UR was collected for InPouch testing, bidirectional gene sequencing of amplicons, and Xpert testing. For “collection only” participating sites, the specimens designated for Xpert testing and reference assay testing were shipped to designated testing laboratories on the same day as collection whenever possible. All Xpert testing was performed within 72 h of collection.

**Assay procedures.** Each trial specimen was collected by using the Cepheid specimen collection device (swab or urine) and tested with the Xpert TV assay. Transport reagent containing the specimen was gently inverted 3 to 4 times, followed by transferring 0.5 ml of the sample to the Xpert cartridge using the transfer pipet supplied. Aptima assay testing was performed according to the manufacturer's package insert. For InPouch testing, CC-VS and ES specimens were inoculated at the collection site. For UR cultures with the InPouch assay, 10 to 15 ml of the urine specimen was centrifuged at  $500 \times g$  for 5 min and the sediment inoculated into the culture pouch on-site within 1 h of collection. Culture pouches were shipped to the reference testing laboratory within 24 h of collection, with receipt of specimens occurring within 48 h of collection. These specimens were shipped at ambient temperature with two warming packs per shipping box. At the reference laboratory, cultures were incubated at 37°C and read daily on weekdays for 3 days to look for the presence of motile protozoans with characteristic morphology according to the InPouch package insert instructions.

The results of the reference tests (InPouch and Aptima for female specimens and InPouch and a validated sequencing method [bidirectional amplicon sequencing of the excess urine remaining from Xpert testing for male specimens]) were used to determine the patient infected status (PIS). The PIS was used to designate a subject as infected or not infected. The subject was considered infected if either of the reference test results were positive for *T. vaginalis*, while the subject was considered not infected

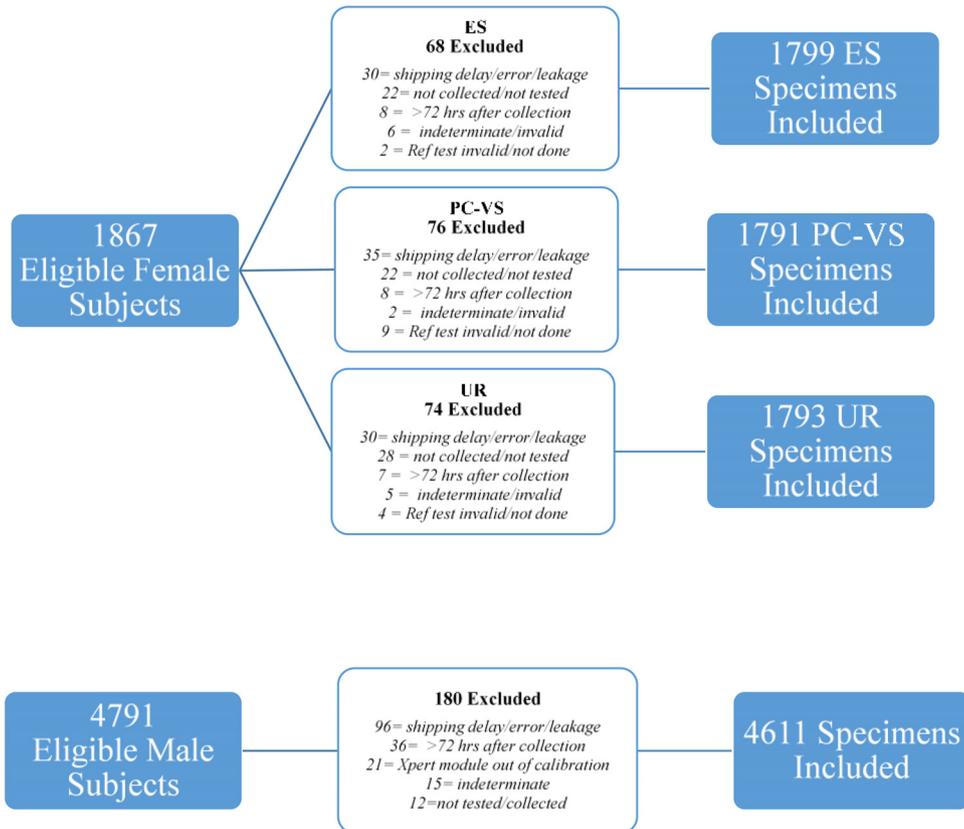


FIG 1 Specimen accountability for specimens from eligible female and male participants. Ref, reference.

when both reference test results were negative for *T. vaginalis*. Bidirectional nucleic acid sequencing was performed on specimens from women with discrepant results between Xpert testing and PIS, as well as an equal number of specimens from women who were determined to be uninfected (i.e., true negatives). For male specimens, secondary sequencing was performed on any specimens with discrepant results between Xpert testing and PIS. Quality control for the Xpert TV assay consisted of one *T. vaginalis*-negative and one *T. vaginalis*-positive external control, with both controls being run on each day that study specimens were tested. Study specimens were not run until valid test results were obtained for both the negative and positive controls. Additionally, several internal controls are built-in to the assay to monitor all aspects of the analytical process with each specimen run, including a sample processing control (SPC), a sample adequacy control (SAC), and a probe check control (PCC). The SPC is present to control for adequate processing of the target trichomonads and to monitor the presence of inhibitors in the PCR. The SAC reagents are included to detect the presence of a single-copy human gene and monitor whether the specimen contains human cells. The PCC verifies reagent rehydration, PCR tube filling in the cartridge, probe integrity, and dye stability. Only those study specimens with valid control results available for all study test methods were included in the data analyses.

Statistical analyses were performed using SAS.

## RESULTS

**Results for female subjects.** A total of 1,876 female subjects were initially enrolled in this clinical study, 1,867 (99.5%) of whom were eligible for inclusion. The nine ineligible subjects consisted of three subjects with a history of hysterectomy, two subjects with improper or incomplete informed consent, two subjects previously enrolled in the study, and two subjects who had been treated with antibiotics within the 21 days prior to study enrollment. Of the 1,867 eligible study participants, 714 (38.2%) were symptomatic and 1,153 (61.8%) were asymptomatic. The average age among eligible study participants was 33.5 years (range, 18 to 78 years).

From the 1,867 eligible female study subjects, 1,799 (96.4%) ES, 1,791 (95.9%) PC-VS, and 1,793 (96.0%) UR specimens were included in the final data set. The reasons for exclusion of each specimen type are shown in Fig. 1.

The Xpert TV (*T. vaginalis*) assay successfully produced results for 98.4% (5,306/5,391) of the samples from eligible female subjects on the first attempt. The 85

**TABLE 1** Xpert TV versus InPouch, Aptima, and PIS results for female subjects<sup>a</sup>

Sample type	Reference test or patient status	Total no. tested	Sensitivity	95% CI	Specificity	95% CI	% prevalence	PPV (%)	NPV (%)
ES	InPouch	1,799	98.7 (153/155)	95.4–99.8	97.6 (1,604/1,644)	96.7–98.3	8.6	89.3	99.9
	Aptima	1,799	100 (175/175)	98.3–99.3	98.9 (1,606/1,624)	98.3–99.3	9.7	90.7	100
	PIS	1,799	98.9 (175/177)	96.0–99.9	98.9 (1,604/1,622)	98.3–99.3	9.8	90.7	99.9
PC-VS	InPouch	1,791	96.9 (156/161)	92.9–99.0	97.7 (1,593/1,630)	96.9–98.4	9.0	80.8	99.7
	Aptima	1,791	97.4 (186/191)	94.0–99.1	99.6 (1,593/1,600)	99.1–99.8	10.7	96.4	99.7
	PIS	1,791	96.4 (186/193)	92.7–98.5	99.6 (1,591/1,598)	99.1–99.8	10.8	96.4	99.6
UR	InPouch	1,793	97.7 (148/150)	95.3–99.8	97.7 (1,606/1,643)	96.9–98.4	8.4	80.0	99.9
	Aptima	1,793	99.4 (178/179)	96.9–100	99.6 (1,607/1,614)	99.1–99.8	10.0	96.2	99.9
	PIS	1,793	98.4 (180/183)	95.3–99.7	99.7 (1,605/1,610)	99.3–99.9	10.2	97.3	99.8

<sup>a</sup>Values in parentheses are the number of true positives over the total of true positives plus false negatives (sensitivity) and the number of true negatives over the total of true negatives plus false positives (specificity). PIS, patient infected status (see Materials and Methods); PPV, positive predictive value; NPV, negative predictive value; ES, endocervical swab; PC-VS, patient-collected vaginal swab; UR, urine.

indeterminate results included 74 ERROR readouts (test failed, possibly because the reaction tube was filled improperly, a reagent probe integrity problem was detected, pressure limits were exceeded, or a valve positioning error was detected), 2 NO RESULT readouts (test was aborted), and 9 INVALID readouts (the SPC [sample processing control] and/or the SAC [sample adequacy control] failed—the sample was not properly processed, PCR was inhibited, or the sample was not properly collected). Eighty-three of the 85 indeterminate cases were retested; two samples were not retested. Seventy-seven of 83 indeterminate cases retested yielded valid results upon repeat assay. The overall rate of assay success was 99.9% (5,383/5,391).

Overall, relative to the patient infected status (PIS) results, the Xpert TV assay demonstrated initial sensitivity and specificity values of 98.4% and 99.7%, respectively, for urine samples, 98.9% and 98.9%, respectively, for endocervical swab specimens, and 96.4% and 99.6%, respectively, for patient-collected vaginal swab specimens (Table 1). There were no statistically significant differences in performance with respect to symptomatic status (Table 2).

Homogeneity analysis by site indicated that the results across sites were poolable for specificity. For diagnostic sensitivity, female ES specimens demonstrated nonhomogeneity; however, the overall sensitivity was high (99.5%), with all sites but one having 100% sensitivity. The one site with less than 100% sensitivity demonstrated a sensitivity of 83.3% ([10/12], 95% confidence interval [CI] 51.6% to 97.9%). Though the

**TABLE 2** Xpert TV versus PIS results by symptomatic status for females<sup>a</sup>

Sample type	Status	No. tested	Sensitivity	95% CI	Specificity	95% CI	% prevalence	PPV (%)	NPV (%)
ES	Symp	685	100 (71/71)	94.9–100	98.5 (605/614)	97.2–99.3	10.4	88.8	100
	Asymp	1,114	98.1 (104/106)	93.4–99.8	99.1 (999/1,008)	98.3–99.6	9.5	92.0	99.8
	Overall	1,799	98.9 (175/177)	96.0–99.9	98.9 (1,604/1,622)	98.3–99.3	9.8	90.7	99.9
<i>P</i> values			0.517	–0.70, 4.48	0.331	–1.69, 0.54			
PC-VS	Symp	682	98.6 (73/74)	92.7–100	99.5 (605/608)	98.6–99.9	10.9	96.1	99.8
	Asymp	1,109	95.0 (113/119)	89.3–98.1	99.6 (986/990)	99.0–99.9	10.7	96.6	99.4
	Overall	1,791	96.4 (186/193)	92.7–98.5	99.6 (1,591/1,598)	99.1–99.8	10.8	96.4	99.6
<i>P</i> values			0.254	–1.04, 8.42	1.000	–0.77, 0.59			
UR	Symp	688	98.6 (71/72)	92.5–100	99.8 (615/616)	99.1–100	10.5	98.6	99.8
	Asymp	1,105	98.2 (109/111)	93.6–99.8	99.6 (990/994)	99.0–99.9	10.0	96.5	99.8
	Overall	1,793	98.4 (180/183)	95.3–99.7	99.7 (1,605/1,610)	99.3–99.9	10.2	97.3	99.8
<i>P</i> values			1.000	–3.25, 4.08	0.655	–0.27, 0.75			

<sup>a</sup>Values in parentheses are the number of true positives over the total of true positives plus false negatives (sensitivity) and the number of true negatives over the total of true negatives plus false positives (specificity). PIS, patient infected status; PPV, positive predictive value; NPV, negative predictive value; ES, endocervical swab; PC-VS, patient-collected vaginal swab; UR, urine; Symp, symptomatic; Asymp, asymptomatic.

**TABLE 3** Xpert TV results versus PIS initial results based on symptomatic status for males<sup>a</sup>

Status	No. of UR samples tested	Sensitivity	95% CI	Specificity	95% CI	% prevalence	PPV (%)	NPV (%)
Symp	1,088	87.5 (28/32)	71.9–95.0	99.8 (1,054/1,056)	99.3–99.9	2.9	93.3	99.6
Asymp	3,523	90.3 (84/93)	82.6–94.8	99.2 (3,401/3,430)	98.8–99.4	2.6	74.3	99.7
Total	4,611	89.6 (112/125) <sup>b</sup>	83.0–93.8	99.3 (4,455/4,486) <sup>c</sup>	99.0–99.5	2.7	78.3	99.7
<i>P</i> values		0.738	–15.8, 10.1	0.020	0.25, 1.06			

<sup>a</sup>Values in parentheses are the number of true positives over the total of true positives plus false negatives (sensitivity) and the number of true negatives over the total of true negatives plus false positives (specificity). PIS, patient infected status; UR, urine; PPV, positive predictive value; NPV, negative predictive value; Symp, symptomatic; Asymp, asymptomatic.

<sup>b</sup>Results from secondary sequencing: 9 of 13 false negatives were *T. vaginalis* negative and 4 of 13 were *T. vaginalis* positive.

<sup>c</sup>Results from secondary sequencing: 27 of 31 false positives were *T. vaginalis* positive and 4 of 31 were *T. vaginalis* negative.

upper CI includes the null hypothesis, the sample size was too small for meaningful analysis. Some site-to-site variation can be expected, as well as some amount of sampling variation. Keeping this site in the pooled analysis, although it may have a slightly lower sensitivity than the other sites, was considered conservative.

**Results for male subjects.** The data in Fig. 1 illustrate specimen accountability for male subjects. A total of 4,798 male subjects were enrolled in the study, of whom 4,791 (99.9%) were eligible for evaluation. The seven ineligible subjects consisted of one subject with improper or incomplete informed consent, two subjects previously enrolled in the study, two subjects who had been treated with antibiotics within the 21 days prior to study enrollment, one subject who was not sexually active, and one subject <14 years of age. The average age among eligible male study participants with valid test results was 36.2 years (range, 16 to 78 years). Of these 4,611 study participants, 1,088 (23.6%) were symptomatic and 3,523 (76.5%) were asymptomatic. The prevalence of *T. vaginalis* in males across all study sites was 2.7%.

In all, a total of 4,626 (96.6%) specimens from eligible male subjects were tested using the Xpert TV assay. The urine specimens excluded consisted of 96 for shipping delays, 36 tested >72 h after collection, 21 GeneXpert modules out of calibration, and 12 not tested. Xpert TV assays for 97.7% (4,521/4,626) of the samples from eligible subjects were successful on the first attempt. The 105 indeterminate results included 84 ERROR readouts, 12 INVALID readouts, and 9 NO RESULT readouts. One hundred of the 105 (95.2%) indeterminate cases were retested; 5 samples were not retested. Ninety of 100 (90%) indeterminate cases that were retested yielded valid results upon repeat assay. Thus, the overall rate of Xpert TV assay success was 99.7% (4,611/4,626).

Overall, relative to the PIS results, the Xpert TV assay demonstrated initial diagnostic sensitivity and specificity for male urine specimens of 89.6% and 99.3%, respectively (Table 3). Secondary sequencing was performed on specimens with discordant results. The validated bidirectional sequencing procedure demonstrated that the sequencing limit of detection (LOD) was similar to the Xpert TV assay male urine analytical LOD, resulting in similar frequencies of random dropouts for specimens with low levels of *T. vaginalis* organisms. There were no statistically significant differences in performance with respect to symptomatic status.

## DISCUSSION

Trichomoniasis is a highly prevalent STD and presents with a spectrum of symptoms or with no symptoms (3). In women, the prevalence of infection spans the reproductive years and beyond, with some studies showing high rates in older women (13). The epidemiology is less well understood in men, although a recent study showed that age over 40 years was also associated with *T. vaginalis*-associated sexually transmitted infections (STIs) (14). Accurate identification of trichomoniasis is important for several reasons, including optimizing treatment, realizing the need for treatment of the sexual partner(s) (15), and the potential for prevention of associated public health consequences, such as preterm birth and the acquisition and transmission of HIV (6–8). The CDC has recently recommended NAAT as the preferred diagnostic modality in light of their superior sensitivity compared to those of direct microscopy or culture-based

methods for detecting *T. vaginalis* (2). Diagnostic testing is recommended for symptomatic women, and screening should be considered for individuals with multiple sex partners, persons who exchange sex for payment, use drugs, and/or have a history of STDs, and women in high-prevalence settings, such as STD clinics and correctional facilities (2). Annual screening is recommended for women with HIV infection due to the high rates of *T. vaginalis* infection in this population (16). Rescreening is recommended within 3 months of the initial diagnosis due to high recurrence rates (17). Currently, there are no firm screening recommendations for men due to the fact that an FDA-cleared test has only recently become available. However, men attending STD clinics should be considered for screening (2). A recent study showed a prevalence rate of nearly 10% among men attending an STD clinic in Birmingham, AL (14).

Although other NAAT in addition to the Xpert TV assay have also recently been FDA cleared for the diagnosis of *T. vaginalis* in women (11, 18), the Xpert TV assay can provide on-demand results in 63 min or less, with early termination for positive results within 40 min. This quicker turnaround time makes the GeneXpert platform ideal for use in high-risk settings where diagnosis and treatment could ideally take place in real time for optimal public health control of this STD.

The platform is easy to use and, thus, suitable for in-clinic testing at the point of care (POC). Furthermore, the equally high diagnostic sensitivities and specificities demonstrated here for urine, self-collected vaginal swabs, and endocervical swabs in symptomatic and asymptomatic patients make the assay an important diagnostic screening tool for patients in high-risk settings like STI clinics and emergency departments, as well as gynecology clinics with laboratory facilities. Of note, the majority of men were asymptomatic, suggesting that screening for trichomoniasis should be considered for high-risk men, such as those attending STD clinics.

The availability of NAAT testing for *T. vaginalis* in men is a welcome addition from a public health perspective and has been a key element missing for the control of this STD. The sensitivity and specificity of the Xpert TV assay relative to the PIS results were both high, 97.2% and 99.9%, respectively. However, it should be noted that InPouch cultures for this study followed the current manufacturer's package insert at the time of the study (Biomed Diagnostics document no. 100-001, revision K), which instructed users to incubate and read cultures for up to 3 days. A study conducted by Rivers and colleagues (19) showed that an additional 17.2% of cultures were identified as positive when cultures were incubated and read up for to 5 days. Thus, a study comparing the Xpert TV assay directly to InPouch cultures incubated for 5 days would need to be conducted in order to determine whether the sensitivity of the Xpert assay would be slightly lower.

In summary, *T. vaginalis* is a highly prevalent STI associated with increased risk of HIV acquisition and transmission, as well as preterm births. The availability of an FDA-cleared test for men is especially welcome. Recent advances in molecular diagnostics for this highly prevalent infection, if implemented, should begin to reduce the burden of disease.

## ACKNOWLEDGMENTS

This study was supported in full by Cepheid, Sunnyvale, CA.

The findings and conclusions in this article are those of the authors and do not necessarily reflect the view of Planned Parenthood of America, Inc. J.R.S. has received consulting fees from Hologic; C.A.G. has received honoraria from Cepheid; S.N.T. has received funding from Becton-Dickinson, Hologic, Cepheid, Beckman-Coulter, EliTech, and Roche.

## REFERENCES

1. Satterwhite CL, Torrone E, Meites E, Dunne EF, Mahajan R, Ocfemia MC, Su J, Xu F, Weinstock H. 2013. Sexually transmitted infections among US women and men: prevalence and incidence estimates, 2008. *Sex Transm Dis* 40:187–193. <https://doi.org/10.1097/OLQ.0b013e318286bb53>.
2. Workowski KA, Bolan GA. 2015. Sexually transmitted diseases treatment guidelines, 2015. *MMWR Recomm Rep* 64:1–137. <https://doi.org/10.15585/mmwr.rr6404a1>.
3. Wolner-Hanssen P, Krieger JN, Stevens CE, Kiviat NB, Koutsky L, Critchlow C,

- DeRouen T, Hillier S, Holmes KK. 1989. Clinical manifestations of vaginal trichomoniasis. *JAMA* 261:571–576. <https://doi.org/10.1001/jama.1989.03420040109029>.
4. Schwebke J, Hook EI. 2003. High rates of *Trichomonas vaginalis* among men attending a Sexually Transmitted Diseases Clinic: implications for screening and urethritis management. *J Infect Dis* 188:465–468. <https://doi.org/10.1086/376558>.
  5. Rivero LR, Pena MR, Perez CS, Monroy SP, Sariago Ramos I, Nodarse JF. 2002. Frequency of *Trichomonas vaginalis* infection in couples with fertility problems. *Rev Cubana Med Trop* 54:85–90. (In Spanish.)
  6. Cotch MF, Pastorek JG, II, Nugent RP, Hillier SL, Gibbs RS, Martin DH, Eschenbach DA, Edelman R, Carey JC, Regan JA, Krohn MA, Klebanoff MA, Rao AV, Rhoads GG. 1997. *Trichomonas vaginalis* associated with low birth weight and preterm delivery. The Vaginal Infections and Prematurity Study Group. *Sex Transm Dis* 24:353–360. <https://doi.org/10.1097/00007435-199707000-00008>.
  7. Hughes JP, Baeten JM, Lingappa JR, Magaret AS, Wald A, de Bruyn G, Kiari J, Inambao M, Kilembe W, Farquhar C, Celum C, Partners in Prevention HSV/HIV Transmission Study Team. 2012. Determinants of per-coital-act HIV-1 infectivity among African HIV-1-serodiscordant couples. *J Infect Dis* 205:358–365. <https://doi.org/10.1093/infdis/jir747>.
  8. Mavedzenge SN, Pol BV, Cheng H, Montgomery ET, Blanchard K, de Bruyn G, Ramjee G, Straten A. 2010. Epidemiological synergy of *Trichomonas vaginalis* and HIV in Zimbabwean and South African women. *Sex Transm Dis* 37:460–466. <https://doi.org/10.1097/OLQ.0b013e3181cfcc4b>.
  9. Borchardt K, Smith R. 1991. An evaluation of an InPouch TV culture method for diagnosing *Trichomonas vaginalis* infection. *Genitourin Med* 67:149–152.
  10. Kurth A, Whittington WL, Golden MR, Thomas KK, Holmes KK, Schwebke JR. 2004. Performance of a new, rapid assay for detection of *Trichomonas vaginalis*. *J Clin Microbiol* 42:2940–2943. <https://doi.org/10.1128/JCM.42.7.2940-2943.2004>.
  11. Schwebke JR, Hobbs MM, Taylor SN, Sena AC, Catania MG, Weinbaum BS, Johnson AD, Getman DK, Gaydos CA. 2011. Molecular testing for *Trichomonas vaginalis* in women: results from a prospective U.S. clinical trial. *J Clin Microbiol* 49:4106–4111. <https://doi.org/10.1128/JCM.01291-11>.
  12. Gaydos CA, Van Der Pol B, Jett-Goheen M, Barnes M, Quinn N, Clark C, Daniel GE, Dixon PB, Hook EW, III, CT/NG Study Group. 2013. Performance of the Cepheid CT/NG Xpert rapid PCR test for detection of *Chlamydia trachomatis* and *Neisseria gonorrhoeae*. *J Clin Microbiol* 51:1666–1672. <https://doi.org/10.1128/JCM.03461-12>.
  13. Ginocchio CC, Chapin K, Smith JS, Aslanzadeh J, Snook J, Hill CS, Gaydos CA. 2012. Prevalence of *Trichomonas vaginalis* and coinfection with *Chlamydia trachomatis* and *Neisseria gonorrhoeae* in the United States as determined by the Aptima *Trichomonas vaginalis* nucleic acid amplification assay. *J Clin Microbiol* 50:2601–2608. <https://doi.org/10.1128/JCM.00748-12>.
  14. Muzny CA, Blackburn RJ, Sinsky RJ, Austin EL, Schwebke JR. 2014. Added benefit of nucleic acid amplification testing for the diagnosis of *Trichomonas vaginalis* among men and women attending a sexually transmitted diseases clinic. *Clin Infect Dis* 59:834–841. <https://doi.org/10.1093/cid/ciu446>.
  15. Soper DE, Shoupe D, Shangold GA, Shangold MM, Gutmann J, Mercer L. 1993. Prevention of vaginal trichomoniasis by compliant use of the female condom. *Sex Transm Dis* 20:137–139. <https://doi.org/10.1097/00007435-199305000-00003>.
  16. Muzny CA, Rivers CA, Austin EL, Schwebke JR. 2013. *Trichomonas vaginalis* infection among women receiving gynaecological care at an Alabama HIV clinic. *Sex Transm Infect* 89:514–518. <https://doi.org/10.1136/sextrans-2012-050889>.
  17. Peterman TA, Tian LH, Metcalf CA, Satterwhite CL, Malotte CK, DeAugustine N, Paul SM, Cross H, Rietmeijer CA, Douglas JM, Jr, RESPECT-2 Study Group. 2006. High incidence of new sexually transmitted infections in the year following a sexually transmitted infection: a case for rescreening. *Ann Intern Med* 145:564–572. <https://doi.org/10.7326/0003-4819-145-8-200610170-00005>.
  18. Van Der Pol B, Williams JA, Taylor SN, Cammarata CL, Rivers CA, Body BA, Nye M, Fuller D, Schwebke JR, Barnes M, Gaydos CA. 2014. Detection of *Trichomonas vaginalis* DNA by use of self-obtained vaginal swabs with the BD ProbeTec Qx assay on the BD Viper system. *J Clin Microbiol* 52:885–889. <https://doi.org/10.1128/JCM.02966-13>.
  19. Rivers CA, Muzny CA, Schwebke JR. 2013. Diagnostic rates differ on the basis of the number of read days with the use of the InPouch culture system for *Trichomonas vaginalis* screening. *J Clin Microbiol* 51:3875–3876. <https://doi.org/10.1128/JCM.02006-13>.